



# Anesthesia 101

Midmark Animal Health Products

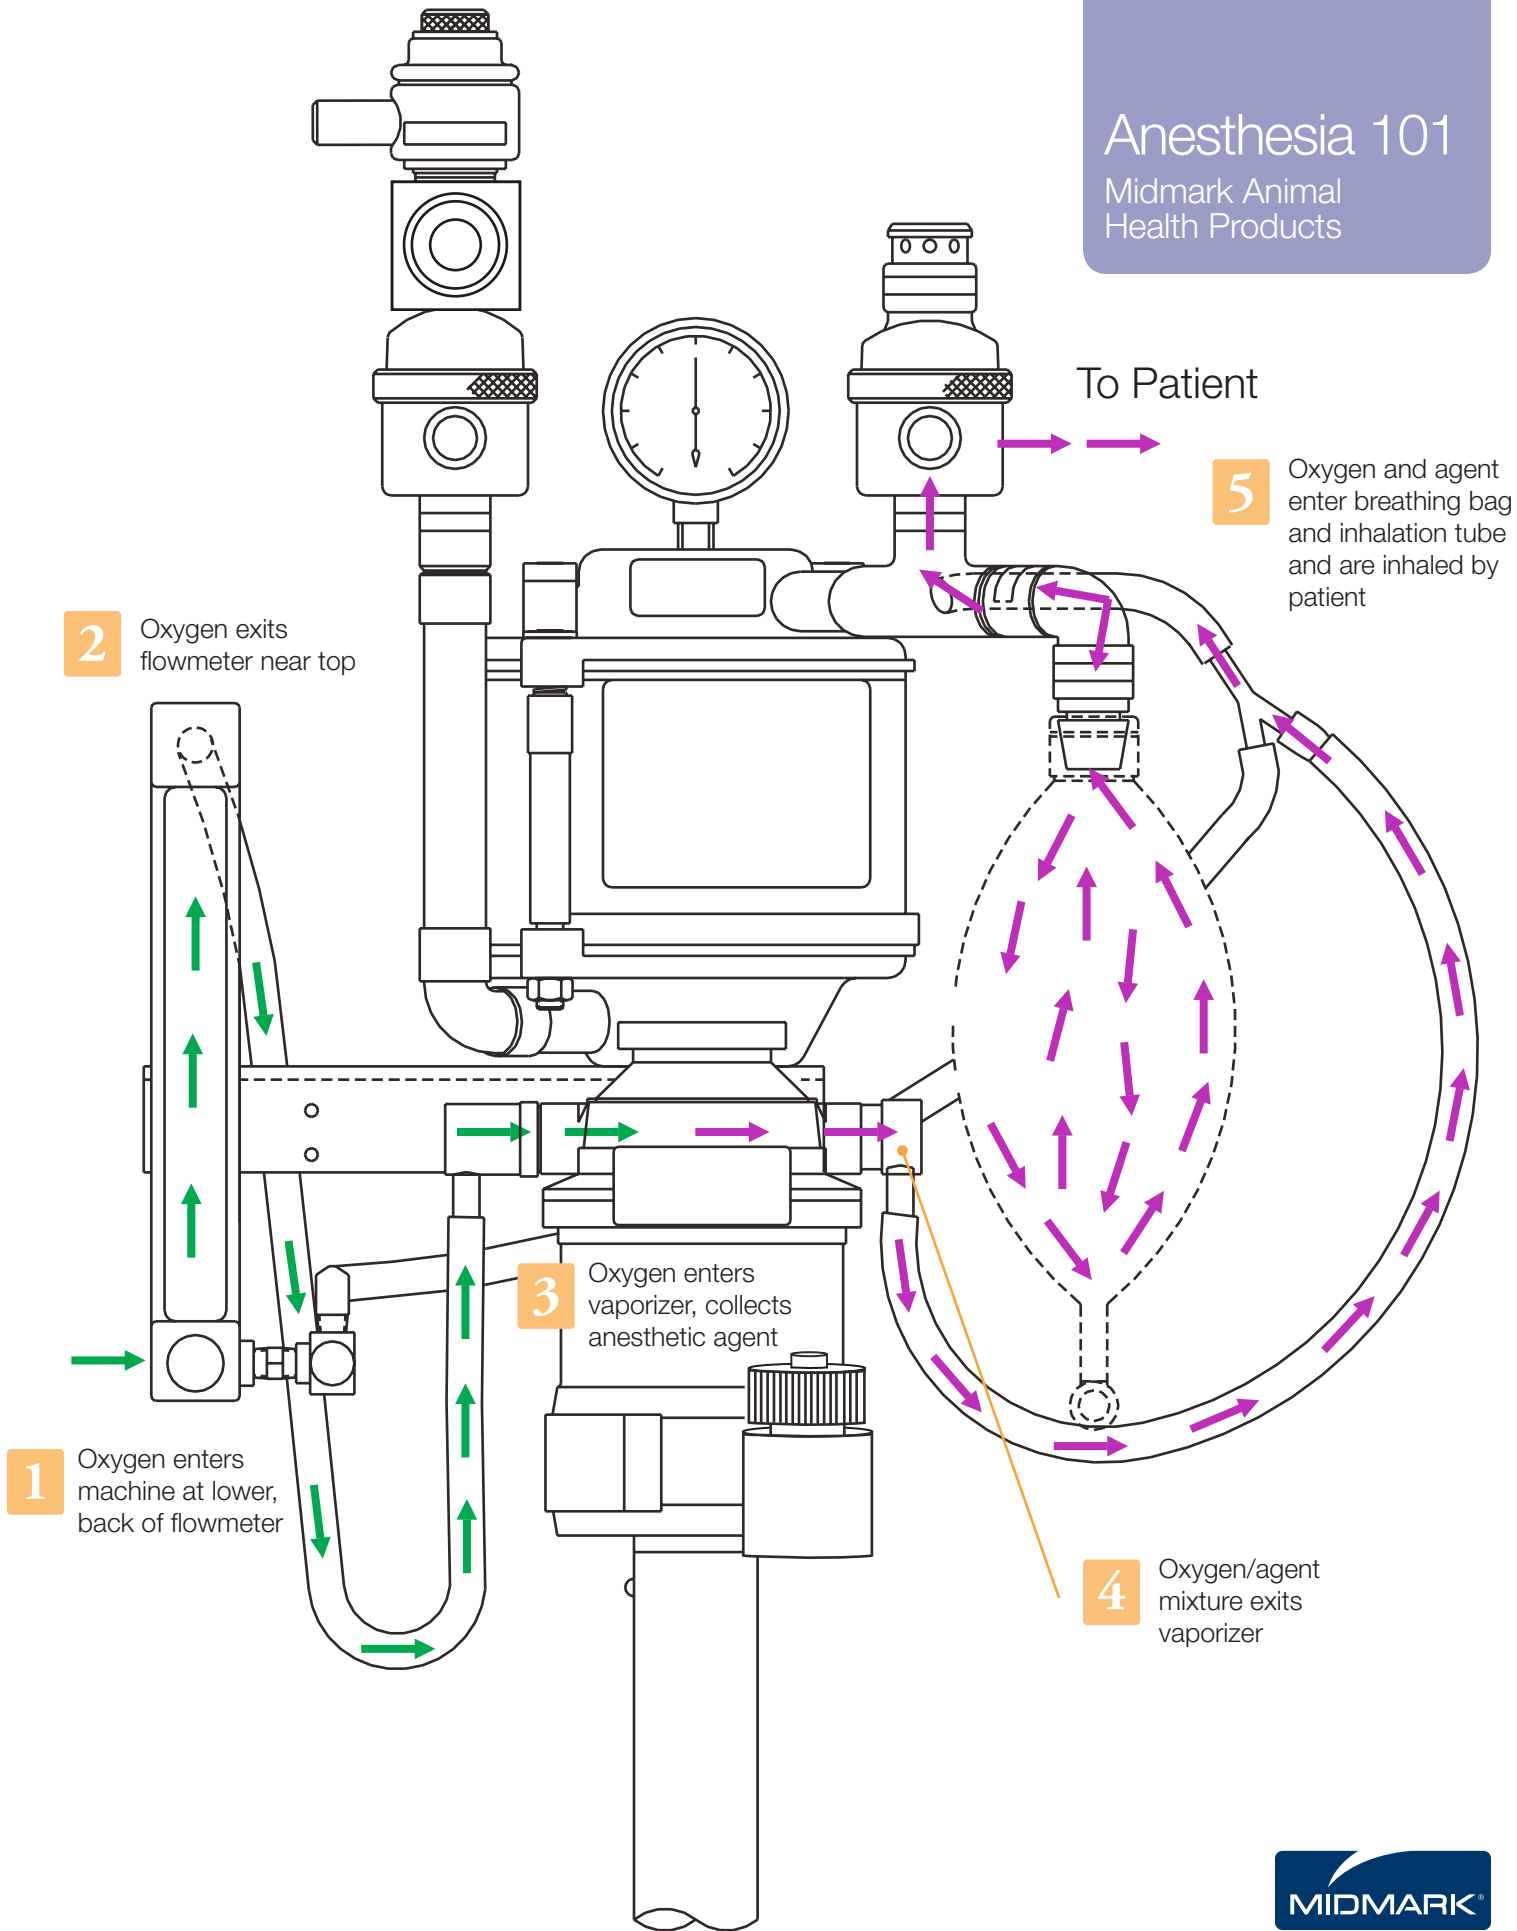

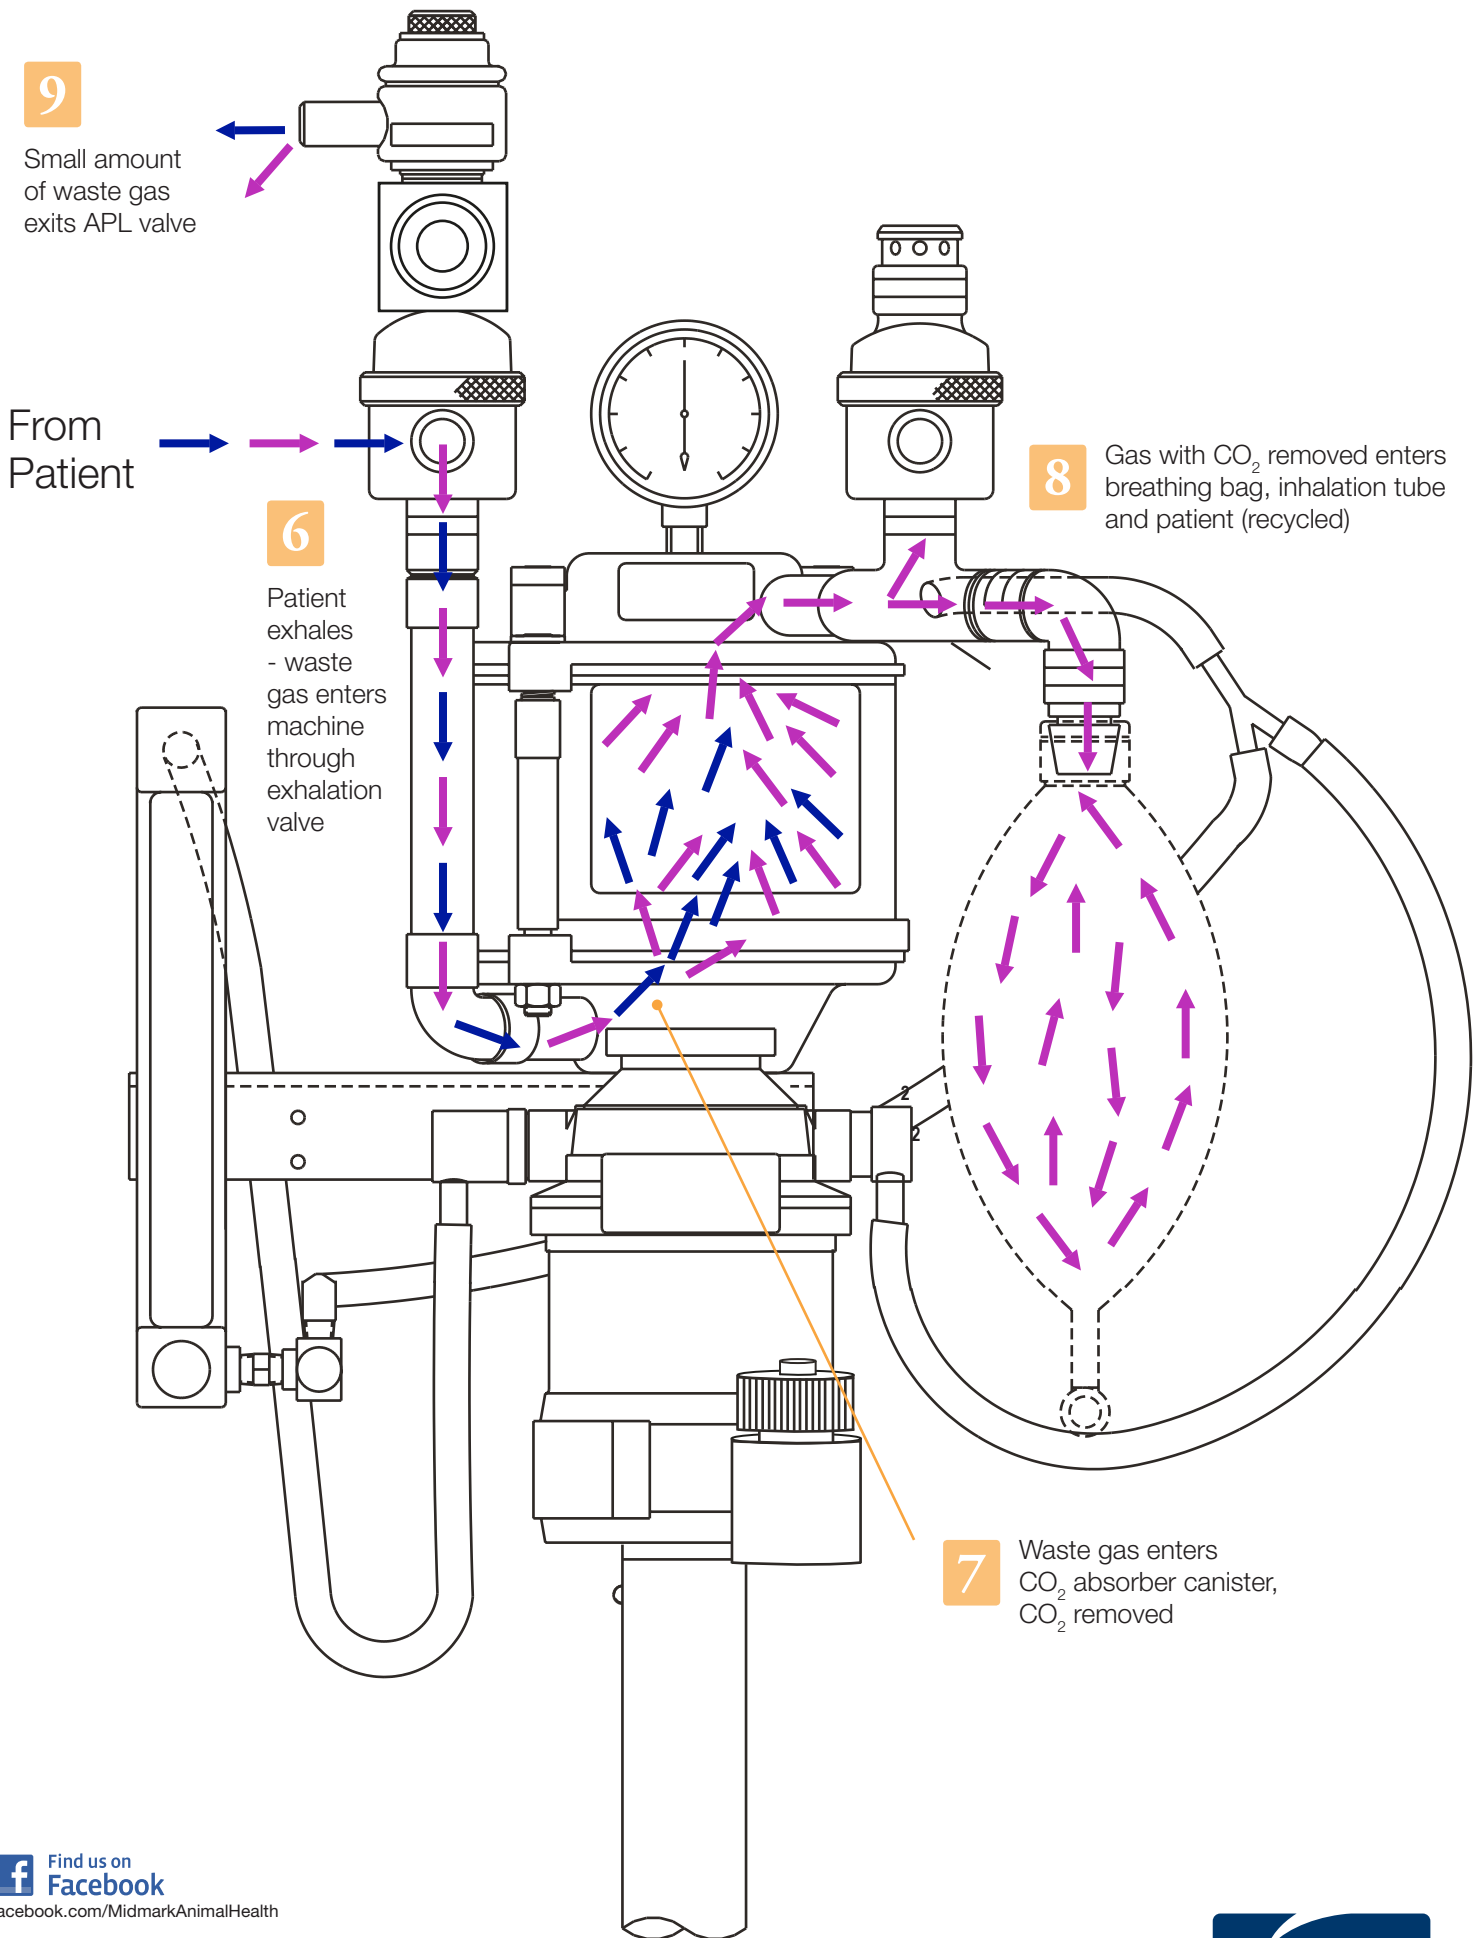

9

Small amount of waste gas exits APL valve

From Patient

6

Patient exhales - waste gas enters machine through exhalation valve

8

Gas with CO<sub>2</sub> removed enters breathing bag, inhalation tube and patient (recycled)

7

Waste gas enters CO<sub>2</sub> absorber canister, CO<sub>2</sub> removed



Find us on Facebook  
facebook.com/MidmarkAnimalHealth

midmarkanimalhealth.com



Because we care.